

Certificate of Analysis

No. CA06081

Product: Eichrom's TRU Resin


Lot #: TRA07066

Eichrom's TRU Resin Lot # TRA07066 has been manufactured according to Eichrom's standard operating procedures. This lot has been tested in accordance with Eichrom's quality assurance policy and procedures. This lot of product meets all Eichrom quality specifications.

ANALYSIS RESULTS

Test Value	Specification	Result
Appearance	White beads	Pass
Distribution Ratio, Eu in 3.1 N nitric acid	≥ 60	88
% ^{241}Am stripped in 4M HCl		
Least acceptable mean (5 rep)	95.0	99.6
Max. standard deviation	2.5	0.4
% ^{241}Am stripped in 0.1M ammonium bioxalate		
Maximum acceptable mean (5 rep)	1.0	0.2
Max. standard deviation	0.5	0.1
% ^{239}Pu stripped in 0.1M ammonium bioxalate		
Least acceptable mean (5 rep)	95.0	97.6
Max. standard deviation	2.5	1.0
% ^{239}Pu stripped in 4M HCl		
Maximum acceptable mean (5 rep)	1.0	0.1
Max. standard deviation	0.5	0.2
Extractant distribution ratio, ^{241}Am strip in 0.05M HNO_3	<0.50	0.31
Raw support resin gravity flow rate, mL/min	0.60-0.80	0.75

TRU Resin Elution Curve

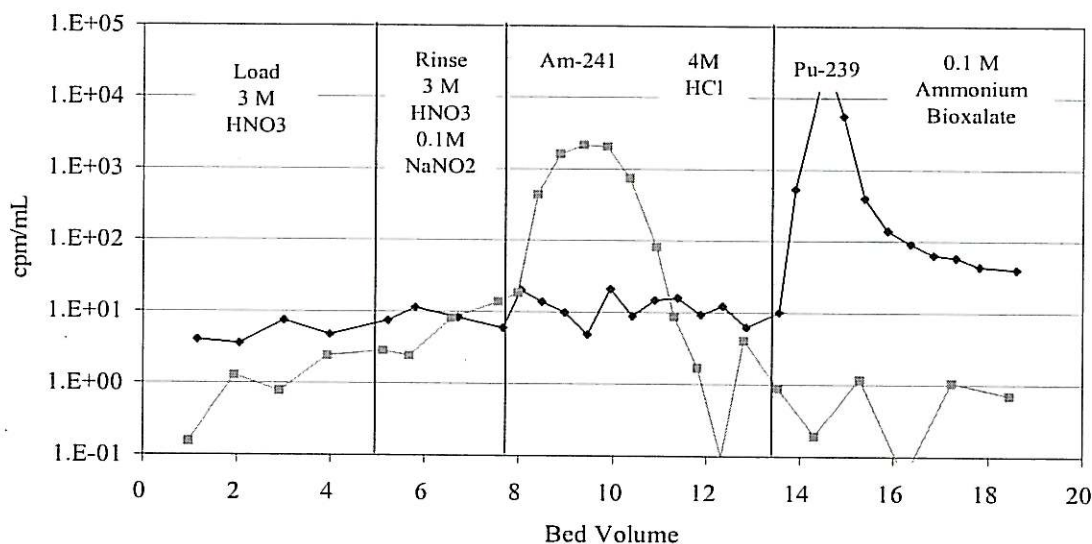

Eichrom recommends the use of gravity flow with 100-150 μm beads, "A" grade.

Joel Williamson
 Joel Williamson
 Senior Quality Control Chemist

Prepared: July 31, 2006