

Certificate of Analysis

No. CA06122


Product: Eichrom's TRU Resin Cartridges
Lot #: TRSR6H

Eichrom's TRU Resin Cartridge Lot # TRSR6H has been manufactured according to Eichrom's standard operating procedures. The lot of resin used to manufacture these cartridges has been tested in accordance with Eichrom's quality assurance policy and procedures. This lot of product meets all Eichrom quality specifications.

ANALYSIS RESULTS

Test Value	Specification	Result
Appearance	White beads	Pass
Distribution Ratio, Eu in 3.1 N nitric acid	≥ 60	90
% ^{241}Am stripped in 4M HCl		
Least acceptable mean (5 rep)	95.0	99.6
Max. standard deviation	2.5	0.2
% ^{241}Am stripped in 0.1M ammonium bioxalate		
Maximum acceptable mean (5 rep)	1.0	0.2
Max. standard deviation	0.5	0.0
% ^{239}Pu stripped in 0.1M ammonium bioxalate		
Least acceptable mean (5 rep)	95.0	95.9
Max. standard deviation	2.5	1.3
% ^{239}Pu stripped in 4M HCl		
Maximum acceptable mean (5 rep)	1.0	0.2
Max. standard deviation	0.5	0.0
Extractant distribution ratio, ^{241}Am strip in 0.05M HNO_3	<0.50	0.31

TRU Resin Elution Curve

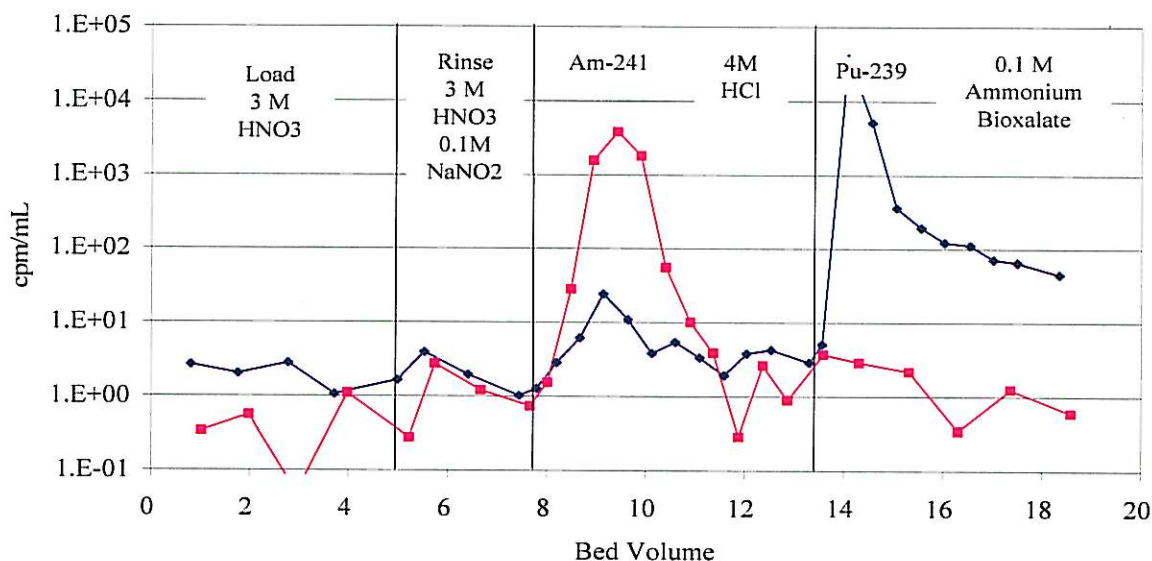

Jill Bryant
Quality Control Chemist

Prepared: December 8, 2006